

X-Ray Effects on Intersil FGA References

Introduction and Background

The Intersil Floating Gate Analog (FGA) technology utilizes a robust stored charge technology borrowed from a standard EEPROM process to produce a precise reference voltage. The stored voltage is the heart of a highly accurate precision voltage reference product. The resulting voltage reference has excellent characteristics which are unique in the industry; very low temperature drift (1ppm/°C), high initial accuracy, and extremely low supply current (<1µA). Also, the reference voltage is not limited to "magic" voltages obtained from bandgap references or buried Zener diodes to achieve temperature drift cancellation.

The floating gate storage cell requires two tunnel diodes to inject charge into a storage capacitor (see Figure 1). The tunnel diodes require high voltage, >10V, to turn on and when unbiased have extremely high impedance and essentially zero charge leakage.

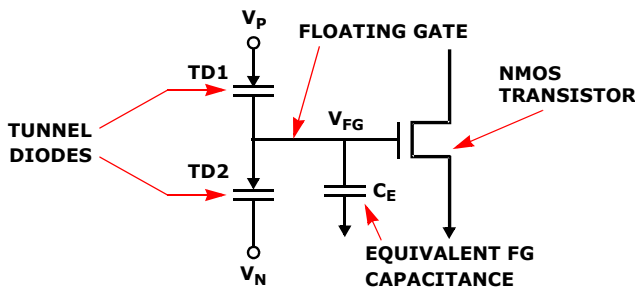


FIGURE 1. FLOATING GATE CELL

The actual voltage reference circuit contains two of the floating gate capacitors and an op amp (see Figure 2). One capacitor sets the common mode voltage and the other sets the output reference voltage. The switches shown in Figure 2 are the tunnel diodes and the V_{CM} and V_{REF} shown are external voltages applied to program the cell at factory test. The output reference voltage is the difference between the common mode and reference

capacitors, which allows output voltage flexibility and adds temperature compensation.

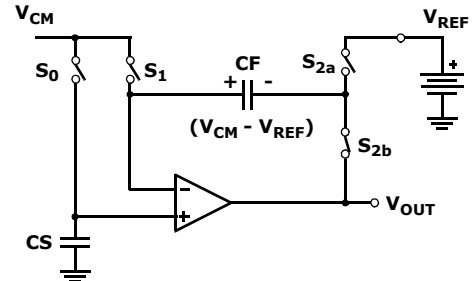


FIGURE 2. FLOATING GATE REFERENCE CIRCUIT SHOWN IN STABLE V_{OUT} STATE

The resulting circuit is highly stable, and the supply current is entirely dependent on the op amp, which can be extremely low current (<1µA) for low power or higher current for low noise applications.

X-Ray Radiation Effects on FGA References

The floating gate capacitor is susceptible to radiation degradation from various particles and photons in excessive doses, as the electrons generated in the silicon dioxide are collected in the storage cell⁶. Normal radiation from cosmic rays or radon which exist in small amounts on earth will not cause the FGA reference voltage to drift appreciably for over 100 years. Artificial sources of radiation such as X-ray machines are capable of high enough doses to cause output voltage shift. Note that Flash memory devices are also susceptible to X-ray radiation degradation, although to a lesser degree as they are not precision analog devices.

Specific threats for X-ray radiation include PC board post-assembly inspection and airport luggage screening. Lesser threats include medical X-ray machines and airport carry-on X-ray.

Some X-ray sources and their equivalent radiation dosage are listed as follows:

- Chest X-ray: 20mrem
- Dental bite-wing X-ray: 140mrem
- Airport carry-on screening: 5mrem to 45mrem
- Airport luggage examination: 5mrem to 2000mrem
- PC board post-assembly inspection X-ray: Typically 10mrem to 200mrem, but due to long observation times can be as high as 700mrem.

X-ray equipment uses 3 main variables to control exposure and therefore dose: tube voltage (usually

kV), tube current (usually 10 μ A to 1mA) and time of exposure (anywhere from <1 second to many minutes). For voltage and current, the larger the number the higher the intensity, and for any of these variables, the larger the number the higher the resulting dose, with other variables fixed. Another variable is the distance from the X-ray emitter to the target or subject. The further from the emitter the less intensity, by 1/distance².

For the purposes of the X-ray effects on FGA references, the main sources we will cover are the Post-Assembly PC Board examination and the Airport screening. Some testing has been completed using assembly X-ray machines and airport X-ray machines with the results presented here.

Intersil FGA X-Ray Testing and Results

Intersil performed testing on FGA reference devices to determine dose levels and output voltage shift for X-ray exposure. The equipment used included the following:

- X-Ray Machine: CR Technology, Bench Top 125, Real Time X-Ray. Voltage Range: 35kV to 125kV, Current Range is 10 μ A to 1000 μ A.
- Dosimeter: RAD-60 by Rados. 55kV to 1MV, 0.1mrem to 999mrem ranges.
- Devices used: ISL21009-50 (5.000V reference) from production stock, no special flow. One device set aside as a control.
- Multimeter: Agilent 3458A.

X-Ray Dose Characteristics

First, the dose from a typical X-ray exposure level was recorded at different exposure times and distances. The results are shown in Figures 3 and 4.

Figure 3 shows the dose is largely proportional to time, and after one minute at 1" distance a dose of 1680mrem

was received. Figure 4 shows the dose varies inversely with distance squared, similar to other radiated sources.

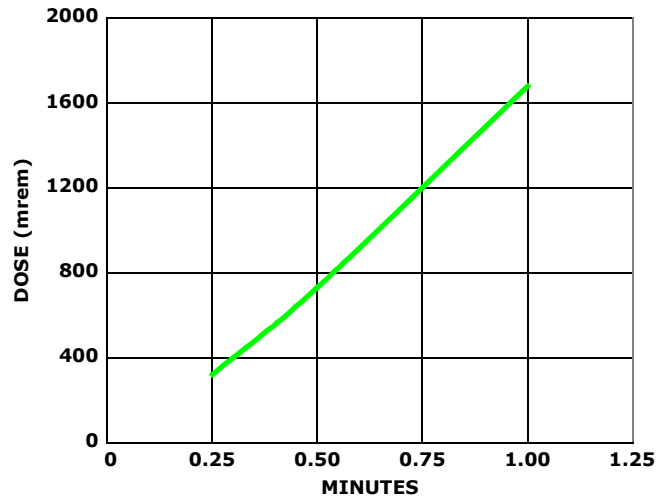


FIGURE 3. DOSE vs EXPOSURE TIME, EXPOSURE = 55kV, 70 μ A, DISTANCE = 1"

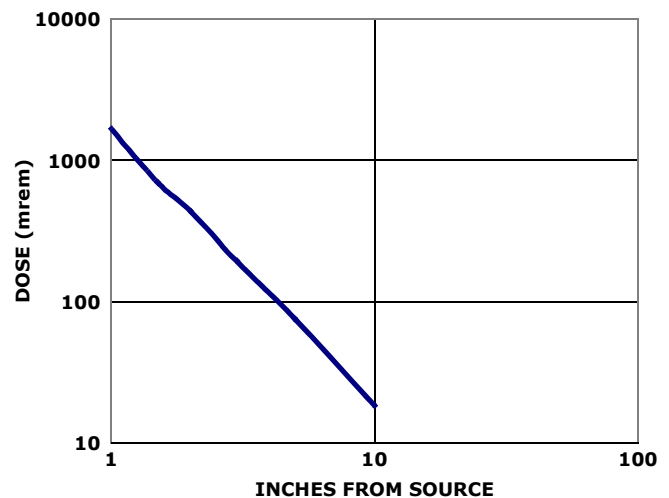


FIGURE 4. DOSE vs DISTANCE, FIXED TIME = 1MIN, LOG-TO-LOG SCALE

Output Shift vs X-Ray Dose Testing

A group of 5.0V reference devices were datalogged and individual devices were exposed at a given intensity (55kV and 70 μ A), at 10" distance with various time periods to vary the received dose. The devices were mounted on the dosimeter to closely approximate the dose received by the FGA. A control device was included to monitor any other shifting or measurement changes, and the control device data is used to adjust the other V_{OUT} Delta results. Table 1 contains the results.

TABLE 1. V_{OUT} SHIFT vs X-RAY DOSE FOR 5V REFERENCE

DEVICE	EXPOSURE DURATION (min)	X-RAY DOSE (mrem)	V _{OUT} DELTA (μV)	DELTA (μV/mrem)	DOSE RATE (mrem/min)
41	1	20.9	-1250	-59.81	20.9
42	2	41.6	-2529	-60.79	20.8
43	3	63.6	-3696	-58.11	21.2
44	4	82.7	-5281	-63.86	20.7
45	6	126.0	-7784	-61.78	21.0
50	None	Control	-57		

Average = -60.87004μV/mrem

TABLE 2. SHIFT vs V_{OUT}

DEVICE	BEFORE X-RAY	AFTER X-RAY	X-RAY DOSE (mrem)	DELTA (μV)	DELTA (%)	EXPOSURE DURATION (MIN)	X-RAY SETTING (kV/μA)
42	4.99991	4.99739	41.6	-2529	0.05	2	55/70
A1	2.50008	2.49918	40.0	-905	0.04	2	55/70
27	5.00006	4.99847	389	-1589	0.03	2	100/30
A2	2.50011	2.49922	416	-887	0.04	2	100/30

The output voltage change with dose did turn out to be a constant, approximately 61μV per mrem (results are dependent on the dosimeter used). Note that 1 minute of X-ray at this level will result in -1.25mV of shift, which placed the voltage reference output well out of spec for accuracy, as specified in the datasheet.

Output Voltage Shift vs Output Voltage

To determine the effect of the actual programmed output voltage, devices from the same product family with different output voltages were exposed to similar doses and the results recorded. For this test, the ISL21009-2.5 and the ISL21009-5.0 were used. Results are shown in Table 2. Two different X-ray settings were used to make sure there is no intensity dependency as well as voltage dependency.

The shift is proportional to the program output voltage, and is constant as a percent of output voltage.

For the lower voltage devices this means less voltage change for the same dose, which could help in some applications where it may be possible to use a much lower voltage.

Filter Testing

For any of the X-ray exposure environments, it is useful to know the properties of filtering materials, or how the most harmful X-ray energy can be reduced and the resulting output voltage shift minimized. Previous testing has been done to determine which materials are most effective for reducing dose ², and Intersil has performed tests to determine which materials reduce device shift.

ZINC FOIL FILTER TESTING

Another group of devices was datalogged. First, a high dose X-ray exposure was done to one device mounted on the dosimeter and produced >10mV shift. Then, a 20mil (0.020”) zinc sheet filter was placed in front of new devices mounted on the dosimeter and the same exposure time and intensity was used on them. A control device was included as well. The results are shown in Table 3.

TABLE 3. V_{OUT} SHIFT USING ZINC FILTER

DEVICE	FILTER	X-RAY SETTING (kV/μA)	EXPOSURE DURATION (MIN)	V _{OUT} DELTA (μV)
46	No	55/70	10	-12,812
47	Zinc	55/70	10	-30
42	No	55/70	2	-2472
48	Zinc	55/70	2	-58
50	Control	55/70	None	-57

The exposure level used was 55kV, 70μA at a 10" distance. The 10 minute exposure was enough to cause -12.8mV shift with no filter. The results with the filter show negligible shift, comparable to that of the control part and is most likely consisting of noise and measurement error. The 2 minute exposure yielded a -2.5mV shift and again, the shielded device had essentially zero shift.

The zinc sheet filter effect is to remove the lower energy X-rays which upset semiconductors and transmit the higher energy X-rays to produce clear images of copper, solder and other metals². Note that no dose information is given since there is still significant levels of radiation measurable with the filter, but it is misleading since the X-ray radiation of interest is actually filtered. Also, the particular dosimeter used is not sensitive to the lower energy X-rays and would not be useful for comparing readings before and after filtering. For reference, the 10 minute exposure, no filter produced 210mrem.

ALUMINUM AND COPPER FOIL FILTER TESTING

Zinc is a very effective metal shield for filtering X-rays in post-assembly analysis, but other metals can be used for general X-ray filtering. Aluminum is used in many cases as an affordable and readily available shield for some applications, but requires significant thickness to be effective. Copper likewise can shield much of the radiation but needs a greater thickness than zinc. Table 4 shows the results of tests using both copper and aluminum shields.

The results show that two 1/2oz copper planes can reduce exposure drift by 8x, which, along with overall reduction in dose, can keep the device well within the output voltage spec.

Aluminum would need to be fairly thick for filtering, requiring about 4x the thickness of copper for the same drift reduction. Since the filtering is proportional to thickness, an 8.5mm aluminum sheet would limit drift

to about 88μV (10x thickness for 10x reduction) at the same exposure stated in Table 4.

TABLE 4. V_{OUT} SHIFT USING COPPER AND ALUMINUM FILTERS

DEVICE	FILTER	X-RAY SETTING (kV/μA)	EXPOSURE DURATION (MIN)	V _{OUT} DELTA (μV)
42	None	55/70	2	-2529
25	850μm Au Foil	55/70	2	-883
51	2 x 1/2oz Cu, 340μm	55/70	2	-472

PACKAGING COPPER LEADFRAME EFFECTS

Note also that the package for the FGA references has a copper leadframe, which is approximately 300μm thick and thus provides similar filtering. Note that the X-rays would need to be directional from under the circuit board for the leadframe filtering to be fully effective, and that most PC boards will have copper planes under the device, providing even more filtering. Table 5 shows results on devices with X-Ray exposure directed from under an FGA device, with and without a PC board and copper ground planes.

TABLE 5. COPPER LEADFRAME AND PC BOARD FILTERING

DEVICE	FILTER	X-RAY SETTING (kV/μA)	EXPOSURE DURATION (MIN)	V _{OUT} DELTA (μV)
21	Leadframe only	55/70	2	-112
18	Leadframe +2 layers ground plane	55/70	2	-44
16	Leadframe +4 layers ground plane	55/70	2	-22
42	Previous direct exposure test result	55/70	2	-2586

These results indicate that a normal PC board with 2 copper planes and an FGA device mounted properly will be extremely resistant to X-radiation from underneath the plane of the board.

Output Voltage Shift vs X-Ray Intensity

X-ray intensity, in tube voltage (kV) and tube current (mA) will affect the rate at which the FGA cell changes voltage. Two devices were exposed to higher tube voltages at 90kV and 100kV while reducing the current to 30μA.

Table 6 shows that the higher voltage actually decreases the drift, and that the lower current decreases drift. This concurs with known effects on semiconductors whereby reducing the tube current will reduce the dose received by the device, and in this case, reduce the voltage drift.

This data makes it clear that when doing X-ray imaging, minimizing tube current reduces FGA device drift.

TABLE 6. OUTPUT VOLTAGE SHIFT vs X-RAY INTENSITY

DEVICE	X-RAY SETTING (kV/ μ A)	DELTA (μ V)	EXPOSURE DURATION (MIN)
34	90/30	-1782	2
27	100/30	-1589	2
42	55/70	-2529	2

Post-Assembly X-Ray Guidelines

As shown in Table Table 1 on page 3, post-assembly x-ray inspection can lead to permanent changes in device output voltage and should be minimized or avoided. Certain actions should be taken to minimize post-assembly X-ray dose. One or more of these will ensure FGA references maintain high accuracy in PC board assemblies.

Use a shield. From the references^{1,2}, many materials can be used for shields, but not all provide effective filtering for charge-storage semiconductor devices. A proven filter (see Table 4) involves placing a 300 μ m zinc foil shield either at the X-ray emission source or over the PC board. The zinc foil acts as a filter to drastically reduce the low intensity radiation which can alter charge storage cells in semiconductor devices, while passing other X-ray energy which produces a useful image for PC board structure analysis. It is also effective to place a small shield over a portion of the board with the FGA device, which may be cumbersome or impossible due to board size or physical construction.

Thick aluminum sheet can be used (10mm or more) to reduce X-ray dose as well, although it may not give the best results for PC board analysis.

Increase the examination distance from the source to the board. Dose decreases as the square of the distance, so maximizing the distance from the X-ray source to the board will minimize the dose.

Reduce the X-ray exposure time. Dose is linearly related to exposure time. Experimental results show that reducing exposure at normal energies from minutes to seconds will preserve the integrity of the FGA voltage reference accuracy.

Reduce the X-ray current level. Dose is nearly exponentially related to the tube current used. Experimental results verified that minimizing the tube current will reduce output voltage shift.

Add voltage reference trimming to the application circuit. For the ISL21009 or ISL21007 products, it is possible to adjust the output voltage with a trim circuit (See [TB473](#)). This will add components to the board, but allows the customer to recalibrate the reference output after all assembly shifts, including reflow (as described in a related application note).

Avoid X-ray exposure. If possible, skip the X-ray inspection and use other methods to verify interconnect bond integrity.

Whatever steps are taken to reduce FGA drift from X-ray inspection, **it is highly recommended that the customer perform a test run on a few boards to monitor the effects at the contract manufacturer so that full production will not be affected.**

Airport Inspection X-Ray Testing

Both Carry-on X-ray machines and the large luggage X-ray machines utilize the same energies as the Post-Assembly X-ray machines, therefore these are also considered as sources of shift for FGA references since products that use the FGA reference may pass through them. Intersil performed tests to evaluate this effect.

CARRY-ON LUGGAGE X-RAY

Table 7 shows the results of a formal experiment with carry-on x-ray on ISL21009 FGA reference devices. The devices were enclosed in an anti-static box in random orientations and carried in a typical computer case. The multiple exposures were from different machines in different U.S. cities to add more variation. The actual dose is unknown, but can be figured from the output voltage shift data previously covered.

TABLE 7. AIRPORT CARRY-ON X-RAY TEST RESULTS

INITIAL VALUE (V)	AFTER CARRY-ON X-RAY: 6x IN 5 CITIES (V)	V _{OUT} SHIFT (μ V)
5.000357	5.000289	-68
4.999935	4.999761	-174
5.000405	5.000307	-98
5.000199	5.000075	-124
5.000239	5.000119	-120
4.999976	4.999877	-99
5.000509	5.000398	-111
4.999998	4.999856	-142
5.000151	4.999952	-199
Average =		-126
Std Dev =		38

The average shift after 6 exposures is comparable to or somewhat less than that from a single IR reflow soldering cycle, ranging from -68 μ V to -199 μ V, and will vary from device-to-device and with orientation in the X-ray machine. The range indicates that device initial accuracy may exceed data sheet specification after multiple exposures. Single exposure will likely not produce significant shift, but a typical product using an FGA reference may be exposed many times in its lifetime.

Calculations show the voltage shift per exposure ranged from -12 μ V to -33 μ V. Assuming the X-ray intensity is similar to the dose testing done previously, it would correspond to a dose from 0.2mrem to 0.6mrem per exposure.

Practical testing has shown the actual doses for a TRX model carry-on X-ray machine are very low, 36 passes resulted in 4mrem of total dose, or about 0.1mrem per pass⁴. These doses are very small so the FGA reference would only be in danger of exceeding the initial accuracy spec after hundreds of passes.

AIRPORT LUGGAGE SCREENING X-RAY

Large airport X-ray machines are now installed at every large airport and are labeled as Explosive Detection Systems or EDS. They use advanced X-ray imaging techniques, similar to medical CAT scans to examine and record the contents of checked luggage. These systems are capable of much higher exposure doses than the carry-on X-ray machines.

The TSA did a survey of airports using these machines and published the results⁴. The testing included total dose data, with tests performed by inserting a dosimeter inside luggage and passing it through the machine 1 or multiple times. They limited the test to two machines that had very different characteristics.

The L3 3DX 6000 uses a helical-cone beam to provide a three dimensional CAT image of an object as it passes along the conveyor. It uses a continuous exposure and scan method which will produce large doses to baggage under X-Ray. The InVision CTX 5500 is a smaller machine which uses a single beam to provide the CAT-slice images. The X-ray detector is only powered when the bag is in the scanning area.

The TSA test results are in Table 8. There is some variability in the dose per pass, and is probably related to the type of luggage used. There is an obvious difference in the dose received from each machine. The L3 with continuous scanning has as much as 30x higher average dose per pass than the CTX 5500.

The effect on the FGA reference can be estimated by using the dose sensitivity stated previously, 61 μ V/mrem. A single pass from a CTX 5500 could produce up to 1.68mV of output voltage shift. The L3 would produce even higher shift, up to 13mV worst case.

TABLE 8. AIRPORT LUGGAGE MACHINE DOSE RESULTS⁴

PASSES	InVision (GE) CTX 5500		L3 COMMUNICATIONS 3DX 6000 EDS	
	TOTAL DOSE MEAN (mrem)	AVERAGE DOSE (mrem/pass)	TOTAL DOSE MEAN (mrem)	AVERAGE DOSE (mrem/pass)
1	7	7.0	156	156.0
3	17	5.7	494	164.7
5	22	4.4	976	195.2
10	280	28.0	2157	215.7

LUGGAGE SCREENING X-RAY TESTING

Intersil performed a test with different FGA products contained in checked baggage and then checked and passed through multiple airport luggage X-ray machines. There was no control over the orientation of the devices or the luggage bag, but no large metallic objects were contained in the luggage. None of the devices showed significant shift, with a measured shift range of -20 μ V to -50 μ V. Although multiple X-ray machines were encountered in this trip, there is no data on which machines were used and no indication that the CAT-scan version with higher intensity was used.

Airport Luggage X-Ray Guidelines

The higher X-Ray dose possible from the airport X-ray machines will definitely cause the reference voltage to shift out of spec from the initial accuracy, especially with repeated exposure. It is advised that FGA references contained in products should not be exposed to luggage X-ray machines if at all possible, or action should be taken to mitigate X-ray effects, as follows.

Provide a warning label. Devices containing FGA references can be labelled as sensitive to X-radiation with an advisory to avoid airport luggage screening.

Shielding and PC board solutions. The FGA package leadframe plus two planes of copper provide an excellent shield for radiation from one direction as shown in Table 5 on page 4. Protection for the device side of the board must also be considered. A shield of zinc foil or sheet, 250 μ m minimum can be placed inside the enclosure above the FGA which effectively filters the most damaging energy. An alternative to consider is a thick aluminum sheet, 10mm or greater, placed over the device side of the PC board.

In applications using multiple PC boards, it is advised to mount a 2-layer (minimum) PC board over the device side of the FGA PC board. If this configuration is used, the protection provided along with a ground plane underneath will effectively shield the device for 50 to 100 passes through an X-ray machine. Since these machines vary in X-ray dose delivered, it is difficult to produce an accurate maximum pass recommendation.

X-Ray Guidelines Update

FGA reference X-ray testing is ongoing and more results will be added when available. Additional data will allow Intersil to provide improved guidelines. For specific applications information dealing with radiation, contact Intersil Applications Engineering.

References

- [1] *Dose Minimization During X-ray Inspection of Surface-Mounted Flash ICs*. Spansion, Inc. Application Note AN01.
- [2] *Filter Optimization for X-Ray Inspection of Surface-Mounted ICs*. Richard C. Blish II, Susan X. Li, and David Lehtonen. IEEE TRANSACTIONS ON DEVICE AND MATERIALS RELIABILITY, VOL. 2, NO. 4, DECEMBER 2002.
- [3] Advisory letter from Agilent Technologies on 5DX X-ray exposure.
- [4] *Evaluation of Radiation Exposure to TSA Baggage Screeners*. Chandran Achutan, PhD, Charles Mueller, MS. Health Hazard Evaluation Report, HETA #2003-0206-3067. Transportation Security Administration (TSA), Washington, DC. September 2008
- [5] United States Patent US 6,751,294; Blish I1 et al., Jun. 15, 2004 PREVENTION OF PARAMETRIC OR FUNCTIONAL CHANGES TO SILICON SEMICONDUCTOR DEVICE PROPERTIES DURING X-RAY INSPECTION. Assignee: Advanced Micro Devices, Inc.
- [6] *Radiation-Induced Soft Errors and Floating Gate Memories*. J. M. Caywood and Reliability Staff. Xicor, Inc. Application Note (not indexed). 1984.

Notice

1. Descriptions of circuits, software and other related information in this document are provided only to illustrate the operation of semiconductor products and application examples. You are fully responsible for the incorporation or any other use of the circuits, software, and information in the design of your product or system. Renesas Electronics disclaims any and all liability for any losses and damages incurred by you or third parties arising from the use of these circuits, software, or information.
2. Renesas Electronics hereby expressly disclaims any warranties against and liability for infringement or any other claims involving patents, copyrights, or other intellectual property rights of third parties, by or arising from the use of Renesas Electronics products or technical information described in this document, including but not limited to, the product data, drawings, charts, programs, algorithms, and application examples.
3. No license, express, implied or otherwise, is granted hereby under any patents, copyrights or other intellectual property rights of Renesas Electronics or others.
4. You shall not alter, modify, copy, or reverse engineer any Renesas Electronics product, whether in whole or in part. Renesas Electronics disclaims any and all liability for any losses or damages incurred by you or third parties arising from such alteration, modification, copying or reverse engineering.
5. Renesas Electronics products are classified according to the following two quality grades: "Standard" and "High Quality". The intended applications for each Renesas Electronics product depends on the product's quality grade, as indicated below.
"Standard": Computers; office equipment; communications equipment; test and measurement equipment; audio and visual equipment; home electronic appliances; machine tools; personal electronic equipment; industrial robots; etc.
"High Quality": Transportation equipment (automobiles, trains, ships, etc.); traffic control (traffic lights); large-scale communication equipment; key financial terminal systems; safety control equipment; etc.
Unless expressly designated as a high reliability product or a product for harsh environments in a Renesas Electronics data sheet or other Renesas Electronics document, Renesas Electronics products are not intended or authorized for use in products or systems that may pose a direct threat to human life or bodily injury (artificial life support devices or systems; surgical implantations; etc.), or may cause serious property damage (space system; undersea repeaters; nuclear power control systems; aircraft control systems; key plant systems; military equipment; etc.). Renesas Electronics disclaims any and all liability for any damages or losses incurred by you or any third parties arising from the use of any Renesas Electronics product that is inconsistent with any Renesas Electronics data sheet, user's manual or other Renesas Electronics document.
6. When using Renesas Electronics products, refer to the latest product information (data sheets, user's manuals, application notes, "General Notes for Handling and Using Semiconductor Devices" in the reliability handbook, etc.), and ensure that usage conditions are within the ranges specified by Renesas Electronics with respect to maximum ratings, operating power supply voltage range, heat dissipation characteristics, installation, etc. Renesas Electronics disclaims any and all liability for any malfunctions, failure or accident arising out of the use of Renesas Electronics products outside of such specified ranges.
7. Although Renesas Electronics endeavors to improve the quality and reliability of Renesas Electronics products, semiconductor products have specific characteristics, such as the occurrence of failure at a certain rate and malfunctions under certain use conditions. Unless designated as a high reliability product or a product for harsh environments in a Renesas Electronics data sheet or other Renesas Electronics document, Renesas Electronics products are not subject to radiation resistance design. You are responsible for implementing safety measures to guard against the possibility of bodily injury, injury or damage caused by fire, and/or danger to the public in the event of a failure or malfunction of Renesas Electronics products, such as safety design for hardware and software, including but not limited to redundancy, fire control and malfunction prevention, appropriate treatment for aging degradation or any other appropriate measures. Because the evaluation of microcomputer software alone is very difficult and impractical, you are responsible for evaluating the safety of the final products or systems manufactured by you.
8. Please contact a Renesas Electronics sales office for details as to environmental matters such as the environmental compatibility of each Renesas Electronics product. You are responsible for carefully and sufficiently investigating applicable laws and regulations that regulate the inclusion or use of controlled substances, including without limitation, the EU RoHS Directive, and using Renesas Electronics products in compliance with all these applicable laws and regulations. Renesas Electronics disclaims any and all liability for damages or losses occurring as a result of your noncompliance with applicable laws and regulations.
9. Renesas Electronics products and technologies shall not be used for or incorporated into any products or systems whose manufacture, use, or sale is prohibited under any applicable domestic or foreign laws or regulations. You shall comply with any applicable export control laws and regulations promulgated and administered by the governments of any countries asserting jurisdiction over the parties or transactions.
10. It is the responsibility of the buyer or distributor of Renesas Electronics products, or any other party who distributes, disposes of, or otherwise sells or transfers the product to a third party, to notify such third party in advance of the contents and conditions set forth in this document.
11. This document shall not be reprinted, reproduced or duplicated in any form, in whole or in part, without prior written consent of Renesas Electronics.
12. Please contact a Renesas Electronics sales office if you have any questions regarding the information contained in this document or Renesas Electronics products.
(Note 1) "Renesas Electronics" as used in this document means Renesas Electronics Corporation and also includes its directly or indirectly controlled subsidiaries.
(Note 2) "Renesas Electronics product(s)" means any product developed or manufactured by or for Renesas Electronics.

(Rev.4.0-1 November 2017)



SALES OFFICES

Renesas Electronics Corporation

<http://www.renesas.com>

Refer to "<http://www.renesas.com/>" for the latest and detailed information.

Renesas Electronics America Inc.
1001 Murphy Ranch Road, Milpitas, CA 95035, U.S.A.
Tel: +1-408-432-8888, Fax: +1-408-434-5351

Renesas Electronics Canada Limited
9251 Yonge Street, Suite 8309 Richmond Hill, Ontario Canada L4C 9T3
Tel: +1-905-237-2004

Renesas Electronics Europe Limited
Dukes Meadow, Millboard Road, Bourne End, Buckinghamshire, SL8 5FH, U.K
Tel: +44-1628-651-700, Fax: +44-1628-651-804

Renesas Electronics Europe GmbH
Arcadiastrasse 10, 40472 Düsseldorf, Germany
Tel: +49-211-6503-0, Fax: +49-211-6503-1327

Renesas Electronics (China) Co., Ltd.
Room 1709 Quantum Plaza, No.27 ZhichunLu, Haidian District, Beijing, 100191 P. R. China
Tel: +86-10-8235-1155, Fax: +86-10-8235-7679

Renesas Electronics (Shanghai) Co., Ltd.
Unit 301, Tower A, Central Towers, 555 Langao Road, Putuo District, Shanghai, 200333 P. R. China
Tel: +86-21-2226-0888, Fax: +86-21-2226-0999

Renesas Electronics Hong Kong Limited
Unit 1601-1611, 16/F., Tower 2, Grand Century Place, 193 Prince Edward Road West, Mongkok, Kowloon, Hong Kong
Tel: +852-2265-6688, Fax: +852-2886-9022

Renesas Electronics Taiwan Co., Ltd.
13F, No. 363, Fu Shing North Road, Taipei 10543, Taiwan
Tel: +886-2-8175-9600, Fax: +886-2-8175-9670

Renesas Electronics Singapore Pte. Ltd.
80 Bendemeer Road, Unit #06-02 Hyflux Innovation Centre, Singapore 339949
Tel: +65-6213-0200, Fax: +65-6213-0300

Renesas Electronics Malaysia Sdn.Bhd.
Unit 1207, Block B, Menara Amcorp, Amcorp Trade Centre, No. 18, Jln Persiaran Barat, 46050 Petaling Jaya, Selangor Darul Ehsan, Malaysia
Tel: +60-3-7955-9390, Fax: +60-3-7955-9510

Renesas Electronics India Pvt. Ltd.
No.777C, 100 Feet Road, HAL 2nd Stage, Indiranagar, Bangalore 560 038, India
Tel: +91-80-67208700, Fax: +91-80-67208777

Renesas Electronics Korea Co., Ltd.
17F, KAMCO Yangjae Tower, 262, Gangnam-daero, Gangnam-gu, Seoul, 06265 Korea
Tel: +82-2-558-3737, Fax: +82-2-558-5338